


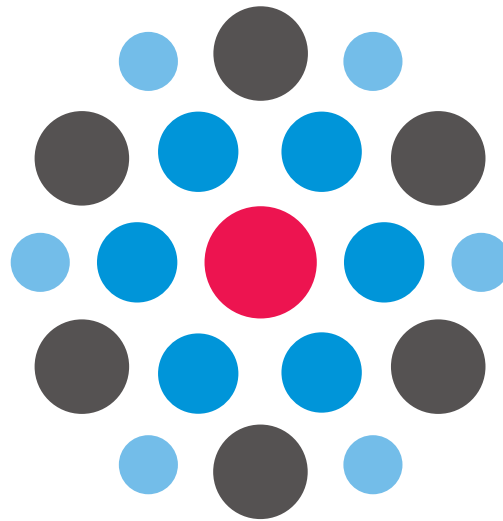

OrthoPulse® lite

User Guide

Contents

1. Introduction

1.1 About OrthoPulse® lite	4
1.2 Intended Use / Indications for Use	4
1.3 Contraindications for Use	6

2. How to Use

2.1 Steps and Schedule for Use	6
2.2 Charging	7
2.3 Status Light Guide	8
2.4 Optional OrthoPulse® lite Software	8

3. Care and Maintenance

3.1 Cleaning	9
3.2 Storage	10
3.3 Service Life	10
3.4 Replacement	10
3.5 Environmental Protection Disposal	10

4. Support

4.1 Orthodontic Treatment	11
4.2 Device Inquiries	11
4.3 Troubleshooting	11
4.4 Warranties	11

5. Safety

5.1 Technical Description and Classifications	12
5.2 Environmental Conditions	13
5.3 EMC Compliance Statement	13
5.4 Electromagnetic Compatibility	15
5.5 Additional requirements for warning and safety notices	18
5.6 Power Adaptor Specification	18
5.7 Warnings and Safety Notices	18

Inside Your OrthoPulse® lite Box


Ensure that all package contents are enclosed and that there is no visible damage

1 OrthoPulse® lite device

2 USB-C charging cable

3 Comfort case

4 Quick Start Guide

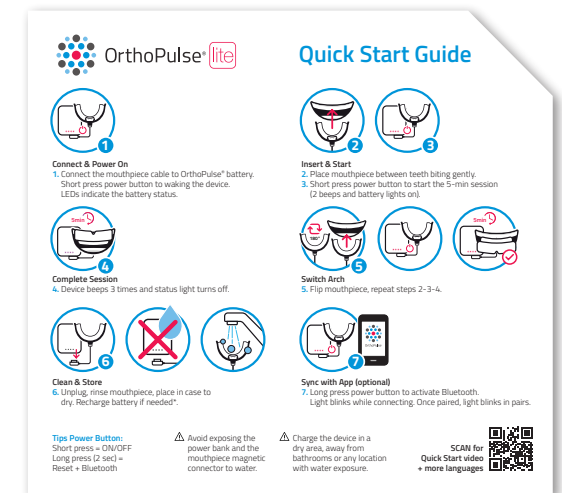

1. Introduction

1.1 About OrthoPulse® lite

OrthoPulse® lite is an established device that uses low levels of light energy to stimulate the bone surrounding the roots of teeth and facilitate tooth movement which may reduce treatment time for braces or clear aligners.

OrthoPulse® lite uses low intensity near-infrared light technology to gently facilitate orthodontic tooth movement.

For further information about the clinical benefits and supporting research, please visit orthopulse.com

OrthoPulse® lite therapeutic device has a mouthpiece with treatment LEDs and a controller unit OP-Battery. The OrthoPulse® lite controller unit has a single-button on/off switch.

1.2 Intended Use /Indications for Use

The OrthoPulse® lite device is intended to accelerate orthodontic movement of teeth and reduce the overall treatment time for the patient. The device is intended to be used in conjunction with traditional orthodontic treatment with brackets and wires or aligners.

The patient should use the OrthoPulse® lite device themselves, following the treatment plan prescribed by their orthodontist or dentist. The OrthoPulse® lite device does not require any servicing or maintenance, the patient shall charge the OP-Battery prior to the first use, and charge it weekly based on battery charge status.

OrthoPulse® lite is operated under prescription by your orthodontist or dentist. Your prescribing orthodontist or dentist will provide instructions on how to use OrthoPulse® lite device.

Please direct questions regarding your orthodontic treatment plan toward your prescribing orthodontist or dentist. Biolux Technology is not authorized and unable to make representations related to patient-specific treatment and/or provide orthodontic treatment advice.

⚠ WARNING: OrthoPulse® lite is a single patient prescription device. Do not use the OrthoPulse® lite appliance on multiple patients. Use by an individual without the proper issuance from an orthodontist may result in unintended consequences, including the possible transmission of viral and bacterial infective agents.

The medical device can be used in any patients if not contraindicated to treat the indications mentioned in section 1.3.

OrthoPulse® lite is an evolution of OrthoPulse®, supported by multiple clinical studies.

Clinical performance claims:

- No increase of root resorption compared to standard orthodontic treatment
- Increased Cellular Metabolism in the Periodontium: PBM at 850 nm increases mitochondrial activity and enhances energy availability (ATP) in periodontal cells.
- Improved Orthodontic Treatment Predictability: PBM improves the predictability of planned orthodontic tooth movements.

Clinical Benefit:

- Patient satisfaction: comfortable treatment that can help reduce discomfort associated with orthodontic treatment
- Reduction of the orthodontic treatment time up to 50 %
- Pain reduction up to 70 %

Clinical Evaluations of OrthoPulse®

Clinical testing of the OrthoPulse® device with orthodontic treatment demonstrated that the device may accelerate tooth movement and may decrease treatment time. Two primary clinical studies of the intra-oral OrthoPulse® demonstrated device performance for its intended use; the device may accelerate orthodontic movement of teeth and may reduce the overall treatment time for the patient when used in conjunction with traditional orthodontic treatment with brackets and wires or aligners.

In a prospective, open-label, randomized cross-over study (TD3), the effect of daily OrthoPulse® use on the rate of orthodontic tooth movement during Invisalign® treatment in the mandibular arch was evaluated. The primary objective was to determine whether OrthoPulse® accelerates tooth movement during the alignment phase. A total of 33 subjects were enrolled, with two later excluded due to unmet inclusion criteria, resulting in 31 participants in the safety population. Of these, 28 had evaluable data for the intent-to-treat (ITT) analysis. Subjects were randomized into two groups: Group A (n=15) began with OrthoPulse®, and Group B (n=13) started without it.

The study's primary endpoint was the mean number of days each Invisalign aligner was worn during control and OrthoPulse® periods. Results demonstrated that aligners were worn for an average of 7.56 days in the control phase and only 5.29 days with OrthoPulse®, a statistically significant reduction of 2.27 days (27.08% decrease; $p=0.00041$). Median values similarly showed shorter wear times with OrthoPulse® (5.50 days) compared to control (7.13 days). For all aligners except Aligner 7—used primarily during the washout phase—the wear time was consistently lower during OrthoPulse® use.

Kaplan-Meier analysis confirmed a consistent leftward shift in aligner wear curves for the OrthoPulse phase, indicating faster progression

through aligners. No serious adverse events were reported. Additionally, clinical monitoring revealed no cases of root resorption, gingival recession, or pathological tooth mobility throughout the six-month observation period. These findings support the safety and effectiveness of OrthoPulse® in accelerating orthodontic tooth movement during aligner therapy.

OrthoPulse® was also evaluated in conjunction with brackets and wires in a controlled study of 33 subjects (mean age 25.0 years). Matched controls (based on subjects' age, initial crowding, eligibility criteria) were retrospectively selected before any data analysis of the OrthoPulse® subjects. Eligibility criteria included requiring that the subjects have permanent dentition, mild to moderate crowding with no labiolingually displaced teeth, Class I or Class II by 1/2 cusp or less, good oral hygiene, and be non-smoking. Subjects who were pregnant, enrolled in another study, had periodontally involved teeth, used bisphosphonates during the study or had spaces between anterior teeth were excluded. There were no differences between groups in terms of gender, ethnicity, age, and initial crowding. The rate of tooth movement was measured using the change in Little's Irregularity Index measurements in both groups to evaluate OrthoPulse® use with fixed orthodontic appliances. Root resorption was determined by use of panoramic dental X-rays collected before treatment and after 6 months of treatment. Results demonstrated that subjects treated with OrthoPulse® showed a statistically significantly faster rate of tooth movement ($p<0.001$) compared to the control group, achieving the primary effectiveness objective of the study. There were no serious adverse events, and no gingival recession or pathological tooth mobility reported throughout the study. Data demonstrated the absence of external apical root resorption with OrthoPulse® use, and that there is no device effect of accelerated tooth movement on tooth root integrity.

Several additional clinical studies were also conducted with prototype and final OrthoPulse® devices to supplement the clinical findings observed in the primary studies, and results consistently confirmed device performance for its indicated use.

Therefore, results from the clinical studies demonstrate that subjects treated with OrthoPulse® achieve statistically significantly faster rates of tooth movement than control. The amount of change in an individual's tooth movement rate during OrthoPulse® daily treatment may be dependent upon their specific biology and treatment plan. For clear aligners, only Invisalign brand aligners have been examined with daily OrthoPulse® use. Results with other brands of aligners may vary.

1.3 Contraindications for Use

- Poor oral hygiene
- Acute oral infection or periodontal disease or oral cancer
- Photosensitivity¹ and photosensitive epilepsy
- Use of drugs that may cause photosensitivity
- Known or suspected allergy or hypersensitivity to device materials

A dental professional should be consulted prior to use if any of these situations are suspected.

2. How to Use

2.1 Steps and Schedule for Use

An OrthoPulse® lite treatment takes five minutes per arch for a total of ten minutes daily.² It is recommended to select the same time every-day to do your treatment.

¹ A condition in which the skin becomes very sensitive to sunlight or other forms of ultraviolet light and may burn easily.

² there are no benefits of doing more than 2 sessions.

The status light guide is available on the bottom of the OP-Battery unit.

Typically, it takes two to three weeks to develop a habit, so be patient. Some patients prefer to set up OrthoPulse® lite next to their bed, so they can do treatments first thing upon rising or prior to sleeping.

Pause Mode:

You may pause your treatment for up to 180 seconds by simply disconnecting the mouthpiece from the power. You will hear a few beeps to let you know that the treatment is paused. To continue, simply reconnect the magnetic connector and short-press the power button — your session will resume right where you left off.

If the pause lasts longer than 180 seconds, the treatment will stop and you will need to restart your OrthoPulse® Lite session.

Pause Mode may also activate if the magnetic connector accidentally disconnects. If this happens, simply reconnect the magnetic connector and short-press the power button — your session will resume right where you left off.

To use your OrthoPulse® lite, complete the six steps below:



1. Remove the OrthoPulse® lite mouthpiece from the shell case, and connect to OP battery via magnetic connector. Press power button to waking the device, OP-Battery LEDs will light up to indicate the battery charge level.




2. Place the OrthoPulse® lite mouthpiece in your mouth, centering it between the front teeth. Bite down gently to hold it in place



3. Press power button to start 5-minutes treatment. The device will beep twice and the status light will turn on indicating that the treatment has started. A warm, pleasant sensation can be felt during treatment. The device has temperature management system, if the temperature exceeds 48 °C the treatment will be paused for cooling, the treatment will be auto resumed after several seconds.
4. Once the treatment is complete, the device will beep three times continuously and the status light will turn off.
5. Flip the device and repeat steps 2 through 4 to treat the other jaw.



6. Unplug the Mouthpiece and wash it after each treatment. Place into the shell case for self-drying. Charge OP-Battery if needed.



TIP: Avoid loud background noise during treatment to ensure you hear the aural indicators.

2.2 Charging

Using the USB cable to connect the OP-Battery to a power adaptor and plug it into a power outlet to charge it. You can use any USB power adapter, e.g. of your mobile phone.

Approximately 6 hours are needed to fully recharge the OrthoPulse® lite OP-Battery. When the device is fully charged, the status light will turn off and the device will sleep automatically.

During the treatment, the device controller (box outside the mouth) could reach a temperature above 41 °C.

Power cable must be removed to start a treatment.

⚠ WARNING: Do not use the device under direct sunlight, or in an environment with ambient temp above 30 °C.

⚠ CAUTION: Place the OrthoPulse® lite on a stable flat surface and out of the way to avoid tripping hazards.

⚠ CAUTION: Charge the device in a dry area, away from bathrooms or any location with water exposure.


⚠ CAUTION: Avoid exposing the power bank and the mouthpiece magnetic connector to water.

2.3 Status Light Guide


Pick up the OrthoPulse® lite to check the status light before your treatment.

Treatment progress

Treatment completion:

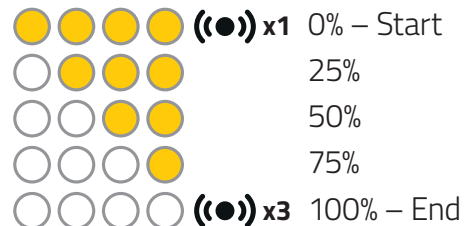


Device beeps 1 time to begin treatment
and 3 times at completion

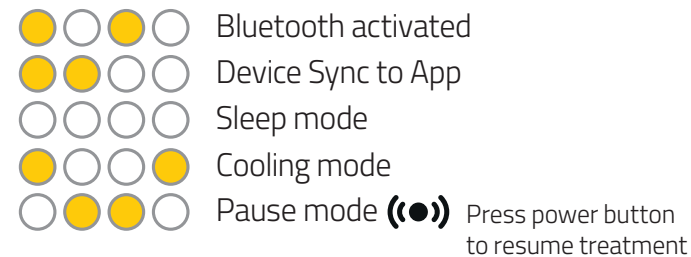

In Charging

Battery charge level:

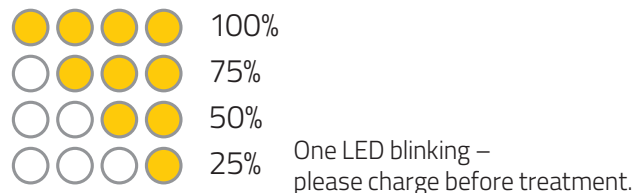

Press and hold power button for
2 seconds to reset the device.

2.4 Optional OrthoPulse® lite Software

This software is no standalone SW and can only be used in connection with OrthoPulse® lite. It has no effect on safety or performance of OrthoPulse® lite but provides an increased scope of features versus the current app in order to digitalize the treatment. Furthermore, it can optionally be used but OrthoPulse® lite can further be used without the software as before.

The main high-level components of the software are the Patient mobile app, the Back-office, the Doctor portal (web) app and the Backend. Those are deployed/distributed through use of the following services: Patient app: Apple App Store for iOS devices and Google Play Store for android devices

Back-office: Cloudfront distribution serving static content from S3 Buckets

Doctor portal: Cloudfront distribution serving static content from S3 Buckets

Backend: Hosted on an EC2 virtual machine: The “Backend System” provides the interfaces to manage the main entities of the software and their sub-entities.

It will be supplied with the following features:

Patient App

- Login (via Email or Phone number)
- Syncing to OrthoPulse® lite hardware
- Treatment status overview
- Streak overview (weekly, monthly)
- Weekly treatment compliance score
- If not in treatment: searching for a doctor close by
- Reminders for weekly sync, daily treatment and aligners change

- Help section with FAQs
- Guides & Manuals on how to use the app and the hardware
- Profile settings
- Display of practice details
- Achievements, e.g. 1-Week streak

Doctor Portal

- Patient management
- adding new patients
- editing patient details
- archiving patients
- displaying patients compliance scores
- displaying communication sent to patient via patient app
- Profile section
- editing personal information
- adding/editing practice information
- adding treatment specifications
- editing reminder texts that are sent to patient via patient app

Backoffice

- Device management
- all device logs
- reporting
- Patient management
- adding new patients
- editing patient details
- archiving patients
- deleting patients
- Doctor management

- adding new doctors
- editing doctor details
- deleting doctor details
- Practice management
- adding new practice
- editing practice
- deleting practice
- Backoffice user management for admins of the backoffice
- Device model management
- Device error code management

The mobile application will be available for all iOS and Android users to be downloaded on the App Store and Play Store respectively for mobile phone usage. A smartphone with either iOS or Android as operating system will be required to be able to download the application from the App or Play Store.

It requires the following minimum operating system specifications:

- iOS minimal Version: 15.7
- Android minimal Version: 9.0 Pie

3. Care and Maintenance

3.1 Cleaning

It is necessary to clean OrthoPulse® lite after every use. It is recommend that patients rinse the mouthpiece under warm water after treatment and set it to air dry on the shell case. Hold the OrthoPulse® lite mouthpiece under the water, avoid water contact on the magnetic connector.

 **CAUTION:** The OrthoPulse® lite device is NOT dishwasher safe.

 **CAUTION:** Avoid rinsing the magnetic connector of the OrthoPulse® lite mouthpiece.

 **CAUTION:** The OP-Battery is not water resistant and should not be rinsed or submerged in water. The charging should be done in a dry environment, inside, and away from water.

3.2 Storage

Store your OrthoPulse® lite mouthpiece in its shell case when not in use. This will prevent damage.

The OrthoPulse® lite device should be stored in a cool, dry place away from direct sunlight. Avoid storing your OrthoPulse® lite, especially OP-Battery in locations where it may be exposed to extreme temperatures.

 **CAUTION:** The OrthoPulse® lite should be stored out of the reach of young children or pets; it is not a toy.

3.3 Service Life

OrthoPulse® lite should last for the duration of your orthodontic treatment. The device should last for up to two years of continuous use if used with care.

The OrthoPulse® lite device contains a lithium polymer battery that will lose charge over time if not re-charged. The OrthoPulse® lite device should be fully charged within three months of delivery and should be fully charged prior to first use. To maintain battery life, do not let the battery completely discharge.

3.4 Replacement

No component of the OrthoPulse® lite device is user- serviceable or replaceable. During the course of treatment, no OrthoPulse® lite components should require replacement. Bite marks and other wear marks that become present in the mouthpiece over time are normal, and do not require replacement. However, they may be indications that you are biting or clenching too hard during your OrthoPulse® treatment. If there are punctures, or any of the internal surfaces of the mouthpiece become exposed, stop using the OrthoPulse® lite immediately and contact support@orthopulse.com.

In case of other damage or unforeseen wear and tear, please contact support@orthopulse.com.

 **WARNING:** Do not tamper with or attempt to repair your OrthoPulse® lite or its OP-Battery unit.

If your OrthoPulse® lite becomes damaged, contact support@orthopulse.com for replacement or repair. Prior to use, inspect OrthoPulse® lite for noticeable signs of damage or wear. Do not substitute any parts or materials in the device.

3.5 Environmental Protection Disposal

The user guide and packaging are recyclable and should be disposed of with other recyclable paper products. To preserve the environment and protect human health, the device should not be disposed of with normal household waste.

Dispose of your device and OP-Battery by delivering them to a designated collection point for the recycling of waste electrical and electronic equipment.

⚠ WARNING: Never incinerate OrthoPulse® lite, expose to excessive heat, short circuit or cause any similar action to the battery. Mishandling the battery may cause burns, fire or explosion.

Contact your local waste authorities, your household waste disposal service or support@orthopulse.com if you require more information regarding disposal.

4. Support

4.1 Orthodontic Treatment

Please contact your orthodontist or dentist directly for all inquiries regarding your treatment.

4.2 Device Inquiries

Please contact the OrthoPulse® lite Support Team:

- for assistance in setting up, using or maintaining your OrthoPulse® lite
- to report unexpected operation or events
- for technical assistance and any concerns specifically related to OrthoPulse® lite or its accessories

Manufacturer Contact Information:

[Biolux Technology GmbH, Neubaugasse 31, 3462 Absdorf, Austria](#)

Email: info@bioluxtec.com

Web: orthopulse.com

4.3 Troubleshooting

Visit the FAQ section on the OrthoPulse® lite website, available here: <http://www.orthopulse.com/patients/support>

4.4 Warranties

Limited Warranty: Biolux Technology (Biolux) warrants to the original purchaser that the OrthoPulse® lite device will be free from defects in material and workmanship for a period of two (2) years from the date of the original purchase from Biolux or its authorized resellers, provided the purchase occurs before the expiration date indicated on the packaging box label of the device. This limited warranty is non-transferable.

If the OrthoPulse® lite device is found to be defective during the warranty period, the purchaser's sole and exclusive remedy, and Biolux's sole obligation, will be, at Biolux's discretion, to either:

1. Repair the OrthoPulse® lite device to conform to its original specifications, or
2. Replace the OrthoPulse® lite device with a comparable product.

Repaired or replaced products or parts may be new or reconditioned and will be covered under this limited warranty for the remainder of the original warranty period.

To obtain warranty service, the purchaser must:

- Contact OrthoPulse® lite support via email at support@orthopulse.com.

This warranty does not cover:

- Defects or malfunctions caused by misuse, neglect, unauthorized attempts to open, repair, or modify the OrthoPulse® lite device.
- Use of the OrthoPulse® lite device with accessories or products not authorized by Biolux.

- Any issues arising from causes other than the intended normal use of the OrthoPulse® lite device.

Any presumption of lack of conformity is expressly excluded.

EXCLUSIONS: TO THE FULL EXTENT ALLOWED BY LAW, THIS LIMITED WARRANTY IS THE PURCHASER'S SOLE AND EXCLUSIVE REMEDY, AND NO OTHER WARRANTIES, CONDITIONS, OR GUARANTEES OF ANY KINDS SHALL APPLY, WHETHER STATUTORY, WRITTEN, ORALLY EXPRESSED OR IMPLIED; INCLUDING WITHOUT LIMITATION WARRANTIES, CONDITIONS OR GUARANTEES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE, PERFORMANCE, QUALITY, OR DURABILITY, ALL OF WHICH ARE DISCLAIMED. IN NO EVENT WILL BIOLUX BE LIABLE FOR ANY SPECIAL, EXTRAORDINARY, INDIRECT OR CONSEQUENTIAL DAMAGES OF ANY KIND WHATSOEVER, INCLUDING WITHOUT LIMITATION DAMAGES FOR LOSS OF DATA, LOST PROFITS, LOSS OF OPPORTUNITY, BUSINESS INTERRUPTION, PERSONAL INJURY OR DEATH, OR ANY OTHER LOSS ARISING OUT OF, RELATING TO, OR IN CONNECTION WITH THE ORTHOPULSE® lite, EVEN IF BIOLUX IS ADVISED OF THE POSSIBILITY OF SUCH DAMAGES.

LIABILITY LIMITATIONS: IF, AS A RESULT OF OR IN CONNECTION WITH ANY USE OF THE ORTHOPULSE® lite, BIOLUX BECOMES LIABLE TO THE PURCHASER OR ANY OTHER PERSON FOR ANY DAMAGES, LOSSES, COSTS, EXPENSES, OR OTHER LIABILITIES WHATSOEVER, AND REGARDLESS OF THE FORM OF ACTION (IN CONTRACT, TORT OR PURSUANT TO STATUTE), THEN BIOLUX'S AGGREGATE LIABILITY WILL BE LIMITED TO AN AMOUNT EQUAL TO THE PURCHASE PRICE PAID FOR THE ORTHOPULSE® lite.

The exclusion of certain conditions and warranties and time limitation of certain liability is prohibited in some jurisdiction, so these limitations and exclusions may not apply to some purchasers. This limited warranty is governed solely by the laws of the Republic of Austria, excluding any rules of private international law or the conflict of laws which would lead to the application of any other laws; the courts of Vienna, 1st district, Austria shall have exclusive jurisdiction over any claims relating to this limited warranty.

Biolux has US and international patents pending for OrthoPulse® lite and the accompanying technology. Patented orthopulse.com/patents The Biolux logo, OrthoPulse® lite, Light Accelerated Orthodontics™, and the collection of these marks are trademarks of Biolux. All rights reserved.

Manufacturers Liability

Biolux Technology assumes no responsibility for any damage, loss, or claims which may result from: failure to follow the instructions contained in this manual; malfunction due to unauthorized repairs or modifications. Use of the OrthoPulse® lite equipment is entirely the responsibility of the operator.

5. Safety

5.1 Technical Description and Classifications

The following is a technical description of OrthoPulse® lite. It is intended to provide all data essential for safe operation, transport and storage as well as permissible environmental conditions and electrical safety classifications.

⚠ WARNING: No modification or servicing of this equipment is allowed.

- OrthoPulse® lite is considered to be an applied part according to the IEC 60601-1 3rd Ed. OrthoPulse® lite is classified as a Type BF applied part.
- Protection Class: Class II equipment.
- OrthoPulse® lite LEDs operate at 850 nm wavelength, 61 mW/cm² output power, corresponding to 18.3 J/cm²

Ingress Protection Class:

- OrthoPulse® lite mouthpiece is rated as IP37, is tool proof and submersible in water up to 1 m deep for up to 30 minutes.

5.2 Environmental Conditions

Environmental Operating Conditions:

- Ambient temperature range: 5°C to 30°C
- Relative humidity range: 15 to 93% non-condensing
- Atmospheric pressure range: 700 to 1060 hPa

Transport and Storage Conditions:

- Minimum ambient temperature: -25°C
- Maximum ambient temperature: 70°C
- Maximum humidity: 93% non-condensing
- Storage pressure range 700 to 1060 hPa

⚠ CAUTION: Ensure the device is not warm after it is charged before starting treatment.

⚠ WARNING: The device shall not be used in conditions beyond the listed above only! The patient shall check the device for any visual defects prior to performing the treatment.

5.3 EMC Compliance Statement

This device has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC rules. These limits are designed to provide reasonable protection against harmful interference in a residential setting. This device generates, uses and can radiate radio-frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this device does cause harmful interference to radio or television reception, which can be determined by turning the device off and on, the user is encouraged to try one or more of the following measures:

- Reorient or relocate the device or the receiver
- Increase the distance between the device and the receiver
- Connect the device to an outlet on a circuit different from that to which the receiver is connected
- Consult the manufacturer or an experienced broadcast engineer/technician for help

Be aware that portable and mobile radio-frequency communications equipment (for example, mobile phones, iPads) may affect the operation of this device; take appropriate precautions during operation.

Accessories

To maintain electromagnetic compatibility (EMC) within limits, the device must be used with the cables and accessories specified by Biolux. The use of accessories or cables other than those specified or supplied may result in increased emissions or decreased immunity of the device.

Radio-Frequency Transmitter

OrthoPulse® lite contains a Bluetooth LE transmitter module that operates at 2.4 GHz. This module is active only when users press On/OFF switch for 5 seconds to activate it. (Possible SW change to activate BLE after each treatment for 10-20 seconds).

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation.

This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.

- Consult the dealer or an experienced radio/TV technician for help

This device complies with part 15 of the FCC rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) This device must accept any interference received, including interference that may cause undesired operation.

Transmitter Module Certifications

CE: Complies with Radio Equipment Directive, RED

2014/53/EU

FCC Limited Modular Certification 15.212 FCC

#2A6CA-OPi

Canada: IC #28421-OPi

Bluetooth SIG certified #D060368

USA – User Information

OrthoPulse® lite contains transmitter module FCC ID:
2A6CA-OPi.

This device complies with part 15 of the FCC rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) This device must accept any interference received, including interference that may cause undesired operation.

 **CAUTION:** Any changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

5.4 Electromagnetic Compatibility

This device is intended for use in a HOME HEALTHCARE ENVIRONMENT. This device emits energy in the infrared range for a predetermined duration.

 **WARNING:** Use of other accessories such as cables other than the ones provided by Biolux Technology for this device may result in increased electromagnetic emissions or decreased electromagnetic immunity of this device and result in improper operation.

 **WARNING:** Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of this device, including cables provided by Biolux Technology. Otherwise, degradation of the performance of this equipment could result.

 **WARNING:** The device automatically stops treatment when a USB connection or charging voltage is detected. This safety feature prevents operation while connected to external power, ensuring user protection against electrical risk.

Exposure to strong electromagnetic sources (80–2700 MHz, up to 10 V/m) and RF wireless communications equipment may cause the device to switch from treatment to cooling mode, with the indicator light flashing continuously.

This temporary condition is safe and expected. Keep the device away from strong EMI sources (e.g., Wi-Fi routers, microwave ovens, TVs, mobile phones).

If flashing persists, turn off or restart the device. Normal operation will automatically resume treatment within 180 seconds after the interference stops.

Electromagnetic Emissions

Test or Measurement	Standards	Test Method	Description	Results
Radiated Emissions	EN 60601-1-2:2015 Ed. 4 CISPR 11 EN 60601-1-11 EN 60601-2-57 EN 301 489-1	ICES-003 Issu.6 Class B Limits	The radiated emissions are measured in the 30-1000MHz range or up to 5x the highest EUT frequency whichever is higher ¹	Complies
Conducted Emissions	V2.1.1 ICES-003 Issue 6 CFR Title 47 FCC Part 15		The Conducted Emissions are measured on the phase and Neutral Power lines in the 0.15 - 30.0 MHz range.	

¹ Highest frequency generated by the device is 2.4GHz

Emission Test	Compliance	Comments
RF Emissions CISPR 11	Group 1	This device uses RF energy only for its internal functions. This device is predominantly intended for use in a HOME HEALTHCARE ENVIRONMENT and to be connected to the PUBLIC MAINS NETWORK
RF Emissions CISPR 11	Class B	
Harmonic Emissions EN 61000-3-2	Class A	
Voltage Fluctuations/ Flicker Emissions EN 61000-3-3	Class A	

Electromagnetic Immunity

Immunity Test	Standard/Test Method	Test Levels	Compliance
Electrostatic Discharge	IEC 61000-4-2	Air Discharge: $\pm 2, 4, 8, 15$ kV Contact Discharge: ± 8 kV	Complies
Radiated RF	IEC 61000-4-3	10V/m, 80% AM @ 1kHz, 30MHz to 2.5GHz, Vertical and Horizontal Polarizations	Complies
Immunity to Proximity Fields from RF Wireless Communications Equipment	IEC 61000-4-3	9 V/m to 28 V/m @ 15 Frequencies 380 - 5800 MHz	Complies
Electrical Fast Transient/ Burst	IEC 61000-4-4	AC Power Lines: ± 2 kV @ 100 kHz Signal Lines: ± 1 kV @ 100 kHz	Complies
Surge	IEC 61000-4-5	$\pm 0.5, 1$ kV line to line, $0^\circ, 90^\circ, 180^\circ, 270^\circ$ $\pm 0.5, 1, 2$ kV line to earth, $0^\circ, 90^\circ, 180^\circ, 270^\circ$	Complies
Conducted RF	IEC 61000-4-6	3Vrms, 0.15-80MHz, 80% AM @ 1 kHz 6Vrms in ISM & Amateur radio bands, 0.15-80MHz, 80% AM @ 1 kHz	Complies
Power Frequency Magnetic Field	IEC 61000-4-8	30 A/m	Complies
Voltage Dips	IEC 61000-4-11	0 % UT; 0,5 cycle at $0^\circ, 45^\circ, 90^\circ, 135^\circ, 180^\circ, 225^\circ, 270^\circ$ and 315° 0 % UT; 1 cycle 70 % UT; 25/30 cycles	Complies
Voltage Interruptions	IEC 61000-4-11	0 % UT; 250/300 cycles	Complies

NOTE: UT is the AC mains voltage prior to application of the test level.

5.5 Additional requirements for warning and safety notices

Side effects that are generally observed with therapeutic light in the near infrared wavelength and which are described in the literature. Even though this type of treatment is generally very safe, negative effects may occur. As a consequence of light therapy, patients can complain of irritability, headaches, eye strain, sleep disturbances and insomnia. Mild visual side effects are not unusual but remit promptly. However, since light therapy is as safe as it is effective, there are no known long-term side effects of this form of light therapy. Other than averting your eyes from the laser's red or infrared light, the FDA has found no other red flags or adverse side effects. Because the light emitted does not cause your skin to burn, there is no risk of pain except under certain conditions.

This is why there are no side effects associated specifically with OrthoPulse® lite. Resulting from the risk analysis, we thus conclude that the OrthoPulse® lite does not contain foreseeable risks of unacceptable levels. The device is designed and manufactured such that, when used as intended, it will not compromise the conditions of safety of the patients and operator, and any remaining risk is managed with a high level of protection of health and safety.

Based on the individual/overall risk/benefit analysis carried out for all identified risks we thus conclude that the OrthoPulse® lite does not contain foreseeable risks of unacceptable levels. The device is designed and manufactured such that, when used as intended, it will not compromise the conditions of safety of the patients and operator, and any remaining risk is managed with a high level of protection of health and safety.

BIOLUX will continue to monitor the risks associated with the use of this product throughout the product lifecycle, including manufacturing,

inspection and testing, complaint handling, non-conformance reports, post-market clinical follow-up, clinical evaluation, post market surveillance, product changes, and management reviews.

5.6 Power Adapter Specification

Standard power adapter with USB-C outlet shall be used to charge the OP-Battery via USB cable; the OP Lite device input is limited to 5.0V / 0.4A.

5.7 Warnings and Safety Notices

United States Federal law and other national regulations restrict this device to sale by or on the order of a doctor. Biolux Technology cannot be held responsible for any damage or injury resulting from a failure to follow the directions in this user guide. Ensure that you are entirely familiar with the correct procedures for operating the appliance before use.

ATTENTION:

- Use only as directed. OrthoPulse® lite must be used under the direction or supervision of an orthodontist or dentist.
- Discontinue use if you have an allergic reaction to OrthoPulse® lite or its accessories and seek medical opinion.
- Chewing or clenching on the bite pad may damage the device, or lead to a choking hazard.
During use, bite gently on the bite pad.
- Staring at the near-infrared light source may cause eye irritation. Do not stare directly at the mouthpiece.
- Avoid knocking, hitting or pulling your OrthoPulse® lite with force. Rough handling may cause damage. Discontinue use if damage is suspected.

- The cable may be a tripping hazard. Plug in near the wall outlet on a stable flat surface.
- Do not use the device while operating machinery or performing complex tasks.
- Do not use with high frequency (HF) surgical equipment.
- Patients with an implanted cardiac pacemaker, defibrillator, or an equivalent cardiac device should not use OrthoPulse® lite unless the cardiac device is known to not be affected by magnetic fields.

Mobile app and OrthoPulse® lite device privacy policy

This Privacy Policy describes the ways in which Biolux Technology (“we,” “our,” or “us”), collects, uses, and discloses information about you through the OrthoPulse® lite and the associated OrthoPulse® lite mobile application (the “OrthoPulse® lite App”). (We refer to the OrthoPulse® lite and the OrthoPulse® lite App collectively as the “OrthoPulse® lite System”.) For using an OrthoPulse® lite or the OrthoPulse® lite App, you have to consent to the processing of your information as set forth in this Privacy Policy, now and as amended by us. Your use of www.orthopulse.com and io.bioluxresearch.com or OrthoPulse® lite Connect™ is governed by a separate privacy policy, which is available here: <https://www.orthopulse.com/privacy-policy> and here, for patients under the age of majority who require guardian/parental consent: <https://io.bioluxresearch.com/admin/doctor/consent/exampleassent>

What Information Do We Collect?

The information we collect from users is an essential component of the OrthoPulse® lite System: Information You or Your Dental Provider Share with Us: We and our service providers collect and store any information that you provide to us, as well as information that is provided to us by your dentist, orthodontist or other treatment

provider. If you, your dentist, orthodontist or other treatment provider create a provider or patient account linked to your name or contact information (an “Account”), we collect the registration information that is shared with us. We collect information when you contact us via the Ortho- Pulse® lite App with a request, question, or comment. We collect information about patients when dental providers create patient Accounts, when patients access their Accounts via the OrthoPulse® lite App, and when an OrthoPulse® lite syncs with the OrthoPulse® lite App. The information provided to us may include, but is not limited to: (a) your name, contact information, email address, mobile phone number, password, OrthoPulse® lite device serial number, and other registration information; (b) your personal details such as your age and gender; (c) orthodontic treatment details such as your treatment start date or planned duration of treatment (d) information regarding your usage of the Ortho- Pulse® lite, such as the date, time, and duration of your use; and (e) information you provide us when you contact us with a request, question, or comment. Even if you, as a patient, do not use the OrthoPulse® lite App, your dental treatment provider may send us information regarding your usage of your OrthoPulse® lite by syncing your OrthoPulse® lite with his or her OrthoPulse® lite App.

Information Automatically Collected From You: We and our service providers collect and store certain types of technical information from your mobile device over time whenever you interact with us through the OrthoPulse® lite App, such as: your Internet Protocol address; your general geographic location (e.g., for purposes of determining your time zone); your mobile device’s model, software version, IP address, and network status; information about how and when you use the OrthoPulse® lite App and/or your mobile device.

How Do We Use This Information?

We may use the information we collect for a number of purposes, including, but not limited to: providing you and your dental provider with information about your use of the OrthoPulse® lite; operating the OrthoPulse® lite System, including providing to you the features and services available through the OrthoPulse® lite App;

- providing you with information, services, or products you request and responding to your inquiries;
- customizing your experience when using the OrthoPulse® lite System, such as by providing personalized treatment options;
- monitoring the safety and efficacy of the OrthoPulse® lite System;
- generating and analyzing statistics about your use of the OrthoPulse® lite System;
- providing you with information about the OrthoPulse® lite System or required notices;
- delivering marketing communications, promotional materials, or advertisements that may be of interest to you;
- improving the OrthoPulse® lite System and the services we provide; and
- detecting, preventing, and responding to fraud, intellectual property infringement, violations of our Terms and Conditions, violations of law, or other misuse of the OrthoPulse® lite System.

Sharing your Information

We may disclose the information we collect from you through the OrthoPulse® lite System in the following circumstances:

Treatment Purposes: Information collected from patients, such as information about usage of the OrthoPulse® lite System, may be disclosed to your dental treatment provider.

Third-Party Service Providers: We may employ other companies and individuals to perform certain business functions on our behalf. Examples include providing data hosting services, application development services, and providing customer service support. These service providers may have access to information that we collect in order to perform services on our behalf.

As Required by Law: We may disclose information in order to comply with legal obligations or requests, such as to comply with a subpoena or other legal process, or to comply with government reporting obligations.

Protection of Rights: We may disclose the information we collect to enforce or apply our Terms and Conditions and other agreements; or protect the rights, property, or safety of the OrthoPulse® lite System, our users, or others. This includes exchanging information with other companies and organizations for fraud protection and credit-risk reduction. This does not include selling, renting, sharing, or otherwise disclosing information that reasonably identifies users for purposes other than those addressed in this Privacy Policy.

In Connection with a Transaction: we may disclose the information we collect to service providers, advisors, potential transactional partners, or other third parties in connection with the consideration, negotiation, or completion of a corporate transaction in which we are acquired by or merged with another company or we sell, liquidate, or transfer all or a portion of our assets.

Where Is This Information Processed?

We process information collected via the Online Services/OrthoPulse® lite App in and subject to the laws of the EUROPEAN UNION, which may not provide the same level protection for your information as your home country. In addition, we may transfer your information outside the European Union to our affiliates, business partners, and service providers located in other countries. By using the Online Services/OrthoPulse® lite System, you consent to such transfer to, and processing in, the European Union, Canada, USA, Switzerland, and Hong Kong.

Information Security

We have administrative, technical, and physical safeguards designed to safeguard the information collected by the OrthoPulse® lite System. However, no information system can be 100% secure, so we cannot guarantee the absolute security of your information. Moreover, we are not responsible for the security of information you transmit to and from the OrthoPulse® lite System over networks that we do not control, including the Internet and wireless networks.

Your Choices

The OrthoPulse® lite App allows you access to information about your Account for the limited purpose of viewing and, in certain cases, updating that information.

Children's Information

If you are a parent or legal guardian of a child that uses the OrthoPulse® lite App, you may be able to review or delete certain information that we have collected in association with your child's use of the OrthoPulse® lite App. If you would like to do so, please contact us at support@orthopulse.com.

Your California Privacy Rights

If you reside in California and have provided to us information that identifies you, you may be entitled to request information once per calendar year about our disclosures of certain categories of certain information to third parties for their direct marketing purposes. Such requests must be submitted to us in writing at the following email address: support@orthopulse.com.

Changes To This Privacy Policy

If we update this Privacy Policy, we will notify you by posting a new Privacy Policy on this page. If we make any revisions that materially change the ways in which we use or share the information previously collected from you through the OrthoPulse® lite System, we may give you the opportunity to consent to such changes before applying them to that information.

Your Rights

You have the fundamental rights to access to information, rectification, erasure, restriction, data portability and to object. If you believe that the processing of your data contravenes data- protection law or your legal claim to protection of your data has been violated in some other way, you can complain to the supervisory authorities.

For Customers in the European Union Reporting of incidents:

All serious incidents related to this product must be reported to the manufacturer and the Federal Office for Safety in Health Care (BASG) at +43 (0)664 831 28 43. A serious incident is defined as an incident which directly or indirectly caused, could have caused or could cause the death or serious permanent deterioration of the health of a patient, user or other person or a serious risk to public health.

The Data Protection Authority is the responsible authority in Austria.
Biolux Technology GmbH
Neubaugasse 31, 3462 Absdorf, Austria
Email: info@bioluxtec.com

Contact Us

If you have any questions about this Privacy Policy or our use of your information collected through the OrthoPulse® lite System, please contact us at support@orthopulse.com.

Manufactured by

Manterra Technologies Inc.
7288 Progress Way
Delta, BC, Canada, V4G 1L4



Manufactured for

Biolux Technology GmbH
Neubaugasse 31, 3462 Absdorf, Austria

Mailing Address

Biolux Technology GmbH
Simmeringer Hauptstraße 397/115, 1110 Vienna, Austria

Registered Address

Biolux Technology GmbH Neubaugasse 31, 3462 Absdorf, Austria

Australian Sponsor

Emergo Australia, Level 20 Tower II, Darling Park, 201 Sussex Street
Sydney, NSW 2000, Australia

Australian Distributor

Kerr Australia Pty. Ltd., Unit 6, 12 Mars Road, Lane Cove West,
NSW 2066, Australia

CH REP CH-REP

Freyr Life Sciences GmbH, Bahnhofplatz, CH-6300 Zug, Switzerland

UK Responsible Person

Freyr Life Sciences Ltd, 9 Greyfriars Road, Reading, Berkshire,
United Kingdom RG1 1NU

Imported and distributed in Europe by

Biolux Technology GmbH
Neubaugasse 31, 3462 Absdorf, Austria

Kerr Italia S.r.l., Via Passanti, 174
Scafati (SA), 84018 Italy
+39 081 850 8311

This Privacy Policy was last updated on 3 March 2021.

GLOSSARY OF APPLICABLE SYMBOLS



Manufacturer




Date of manufacture




Direct current



Class II Equipment



Environmental temperature limit for use



Shipping and storage temperature range



Keep Dry



Fragile, handle with care



Expiration date



Federal law restricts this device to sale by or on the order of a doctor



Serial number



Catalog Number



General Caution Sign



Follow the instructions



Refer to instruction manual




Type BF Applied Part



Humidity Limitation



Separated collection for electrical and electronic equipment use



Device has 10 minutes treatment time, 24 hours Off time



Single patient multiple use



Medical device



Swiss authorized representative

The label with the respective symbols is attached on the charging case.



Certified by TUV

Complies with
IMDA standard
DA107947


OrthoPulse lite
Model Number OPiL-100
UDI-Di: 91201180900032

Complies with FDA regulation

© 2026 Biolux Technology. All rights reserved.
OrthoPulse® and all other Biolux product names and slogans are trademarks and registered trademarks of Biolux.

TD-IFU-EN_OrthoPulse_V1.2
Released on 17 SEP 2026

Questions?
orthopulse.com



OrthoPulse® **lite**