# Count on Cell-Chex to Comply with ISO 15189

*Originally published in Leading Edge* **Autumn/Winter 2016**


ISO 15189 applies to all laboratory methods provided by accredited laboratories, and this includes methods that provide a manual assessment. Using 3rd party verified controls provides greater confidence in test system results.

The Cell-Chex control from Streck Laboratories provides a manual, procedural control for a laboratory standard operating procedure to assess body fluids (synovial, pleural, pericardial, peritoneal and cerebrospinal fluid samples) for the abnormal presence of cells and artefacts, such as Red Blood Cells (RBCs), White Blood Cells (WBCs) including a 5 part differential count, Urate Crystals (UC) and calcium pyrophosphate dihydrate crystals (CPPD). The control is available with three vial options, Level 1 with urate crystals, Level 1 with CPPD crystals and Level 2 with higher cell counts and no crystals, giving the laboratory the ability to choose the best control for the type of body fluid to be assessed.


**Cell-Chex has Urate Crystals (L1-UC) and CPPD Crystals (L1-CC)** *(Shown right)*

An automated body fluid control is also available in 3 levels for those haematology analysers that can enumerate red and white blood cells at these low levels in body fluids.


L1-UC Hemacytometer

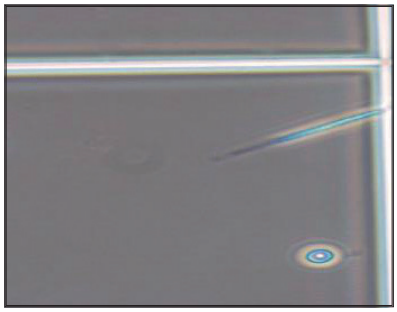


L1-CC Hemacytometer

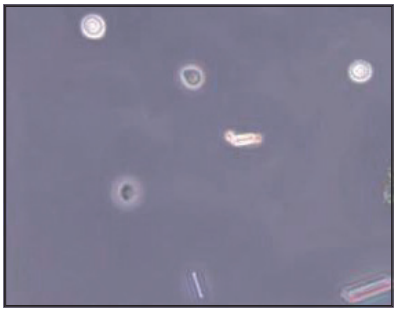

L1-UC Cytocentrifuge

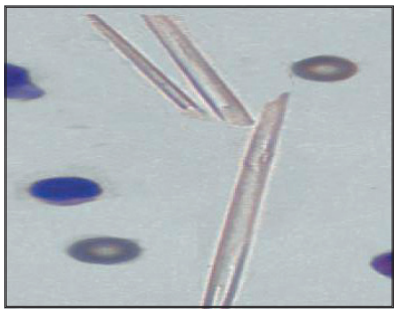


L1-CC Cytocentrifuge

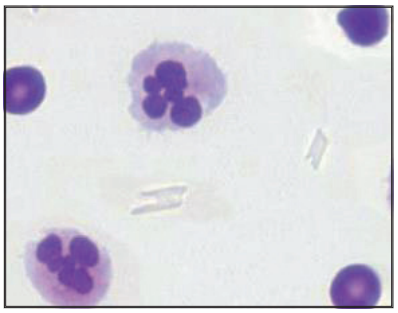

L1-UC Polarizing Scope



L1-CC Polarizing Scope

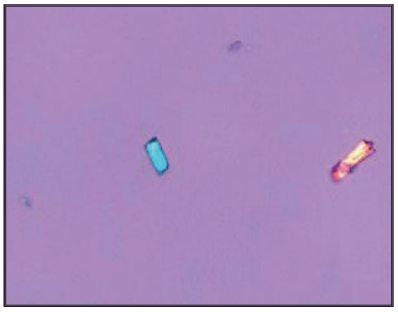

For more information on Cell-Chex and Cell-Chex Auto please visit our website at **www.alphalabs.co.uk/cell-chex**

alpha laboratories
Email: sales@alphalabs.co.uk
Web: www.alphalabs.co.uk